

4-STAGE ULTRA CLEAN WATER SYSTEM



User's Guide

Please Read Before Installing & Using this Equipment



15531 - 24th Avenue, Unit 24, Surrey, BC V4A 2J3 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538 - 1295

CONTENTS
FEATURES AND BENEFITS 4
BEFORE YOU BEGIN Installation Tools Required
INSTALLATION INSTRUCTIONS
Installation Instructions
Installation Diagram 8 Faucet Installation 9
USAGE INSTRUCTIONS
Protocol for Usage
Changing your Cartridges - Instructions11
Connecting & Disconnecting Cartridges
Maintenance Supplies
Optional Features
GUARANTEE/WARRANTY
INTRODUCTION TO WATER QUALITY
Potable Water Quality & Contamination Parameters
Source of Water Contaminants
Primary Parameters
Microbiological Guidelines
Chemical & Physical Guidelines
Secondary Parameters

	10
Chlorination of Public Drinking Water Systems	
Secondary Parameters	19
Turbidity & Hardness	19
Pharmaceutical Grade Water	
Using the Ezee Kleen 2.5 HD to Control Water Quality	20
Invasive Procedures & Universal Precautions	
Contained Dental Unit Waterlines	21
Steam Sterilization of Dental Instruments	
Ultrasonic Baths, Instrument Cleaning & Film Developers	
Function of the Ezee Kleen 2.5 HD	
Comparative Assessment for the Removal of Various Water Pollutions	
Effectiveness of Ultraviolet Radiation Against Different Organisms	
Analytical Report on Ezee Kleen 2.5 HD Water Quality	

4 - STAGE ULTRA CLEAN WATER SYSTEM Model: 8000

FEATURES AND BENEFITS

PRESENTING FOUR STAGES OF WATER PURIFICATION IN ONE SIMPLE SOLUTION

STAGE 1: Prefiltration removes color, odor, taste and suspended solids

- STAGE 2: Reverse osmosis removes up to 98% of all organic and inorganic substances
- STAGE 3: De-ionization removes all remaining dissolved solids
- STAGE 4: Ultraviolet radiation reduces any harmful organisms

FEATURES

- Produces 1 gallon (4 litres) of autoclave-safe water in 4 minutes!
- Reduces suspended solids (organic & inorganic)
- Produces onsite, water of the quality necessary to comply with all autoclave manufactures TDS level guidelines (less than 2.5 PPM of dissolved solids)
- Self monitors (unlike bottled water)
- Ultraviolet (UV) radiation reduces bacteria, viruses and other microorganisms
- Reduces microbial contaminants
- Under counter installation with designated dispensing faucet at sink

APPLICATIONS

- Autoclaves
- Contained dental unit waterline systems

BENEFITS

- Ultra clean water on demand
- Ensure you never run out of water for your autoclaves
- Eliminate last-minute store runs for water
- Eliminate bulky storage of bottles
- Consistent water quality less than 2.5 PPM
- Reduce maintenance & equipment failure
- Out of sight
- Save money!



15531 - 24th Avenue, Unit 24, Surrey, BC V4A 2J3 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538 - 1295

© 2009 - 2024 Oasis Dental Group Inc.™

BEFORE YOU BEGIN

Installation Tools Required:

- multi purpose screw driver
- electric drill
- 1" and 3/8" drill bit
- crescent wrench
- sharp utility knife
- pliers
- teflon tape

Check to be sure you have all the following parts or components:



EZEEKLEEN 2.5 HD Unit (12"w x 16"h x 6"d)

- Prefiltration cartridge
- Reverse Osmosis cartridge
- Ultraviolet cartridge
- De-ionization cartridge
- Water Quality Monitor Power Source: 2 x AA Batteries




8.5" height
6" reach



UV Cartridge Power Supply

BEFORE YOU BEGIN

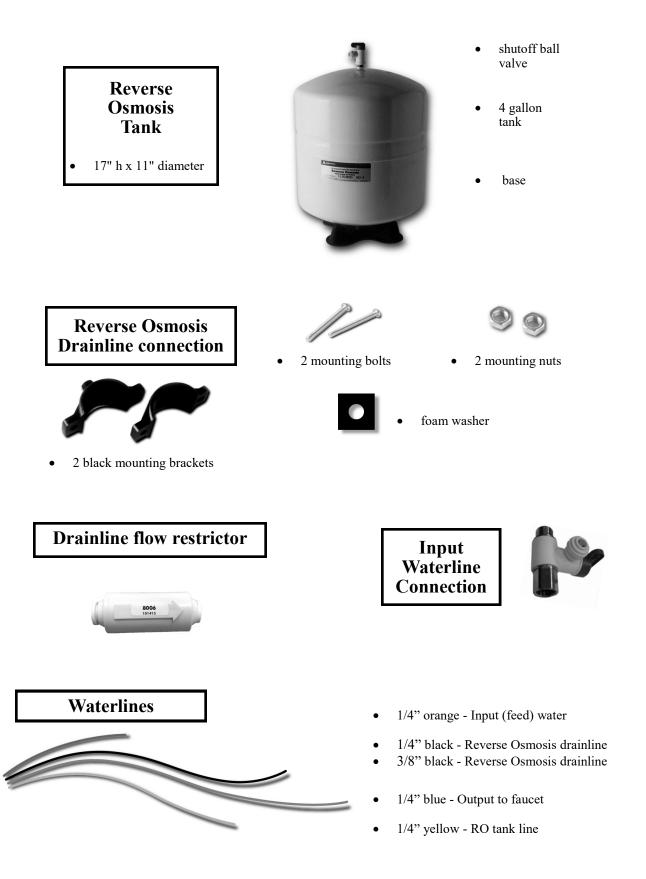

4-STAGE ULTRA CLEAN WATER SYSTEM

Model: 8000

INSTALLATION INSTRUCTIONS

READ INSTRUCTIONS BEFORE COMMENCING INSTALLATION

- 1. Ensure unit is complete with all componentry
- 2. Beneath sink, turn off cold water at the shut off valve
- 3. Determine most suitable place to mount unit (ideally mount unit on left or right side of sink cabinet wall near the front (unit will free stand do not fasten to the wall) allowing for removal for periodic maintenance)
- 4. Determine most suitable place for RO tank-ideally back corner of sink cabinet
- 5. Ensure power supply is within reach of unit and electrical receptacle
- 6. Determine most suitable place to mount faucet in countertop (allowing water to flow into sink-you will be drilling a 7/8" hole)
- 7. Ensure cold waterline is within reach of unit
- 8. Ensure sink drain pipe is within reach of unit
- 9. Install faucet in countertop (use "Faucet Installation Instructions" page 9 in this manual)
- 10. Determine most suitable place to connect drain pipe making sure this connection is easily accessible for routine maintenance

drill 3/8" hole in drain pipe mount foam washer on inside of drain pipe bracket connect mounting brackets (2) to drain pipe with bolts/nuts tighten mounting bracket with bolts/nuts

- 11. Connect universal angle stop connection valve to cold waterline angle stop valve use teflon tape remove cold water riser waterline from top of angle stop valve install universal connection valve to top of angle stop valve connect cold water riser waterline to top of universal connection valve
- 12. Install ball shutoff valve on tank use teflon tape on tank screw thread
 - place tank on mounting base

place tank in back corner of sink cabinet

- 13. Place unit free standing with it's back to either the left or right side cabinet wall undersink (this allows the unit to be removed and laid on it's back in front of the sink cabinet for periodic maintenance)
- 14. Connect all waterlines to unit
 - connect 1/4" blue faucet waterline to faucet stem using 1/4" quick connect fitting and to unit
 - connect 1/4" yellow tank waterline to tank and to unit
 - connect 1/4" black drain line from faucet to unit
 - connect 3/8" black drain line from faucet to drain pipe connector

connect 1/4" orange supply waterline to universal angle stop connection valve and to unit

15. Shorten waterlines to appropriate length - allow enough length to remove unit and set on its back in front of sink cabinet for periodic maintenance - when cutting tubing make sharp, square cuts

Shorten 3/8" black drainline so that it has a reasonably direct vertical drop to drainpipe as it is gravity fed


- 16. Install drainline flow restrictor on 1/4" black drainline about 6" from unit (on outside of unit)
- 17. Turn on cold water
- 18. Bleed air from system by keeping tank closed and faucet open flow from faucet will be a slow trickle (5 oz/minute)
- 19. Check for leaks close faucet to maximize pressure on system
- 20. Auto shut off valve can be tested by closing and opening faucet drainline flow should stop shortly after closing faucet with tank closed and should re-open when faucet is opened
- 21. Plug in power supplies for ultraviolet cartridge and monitoring system
- 22. Open tank valve and allow 2 hours for RO tank to fill



4-STAGE ULTRA CLEAN WATER SYSTEM

Model: 8000

INSTALLATION DIAGRAM

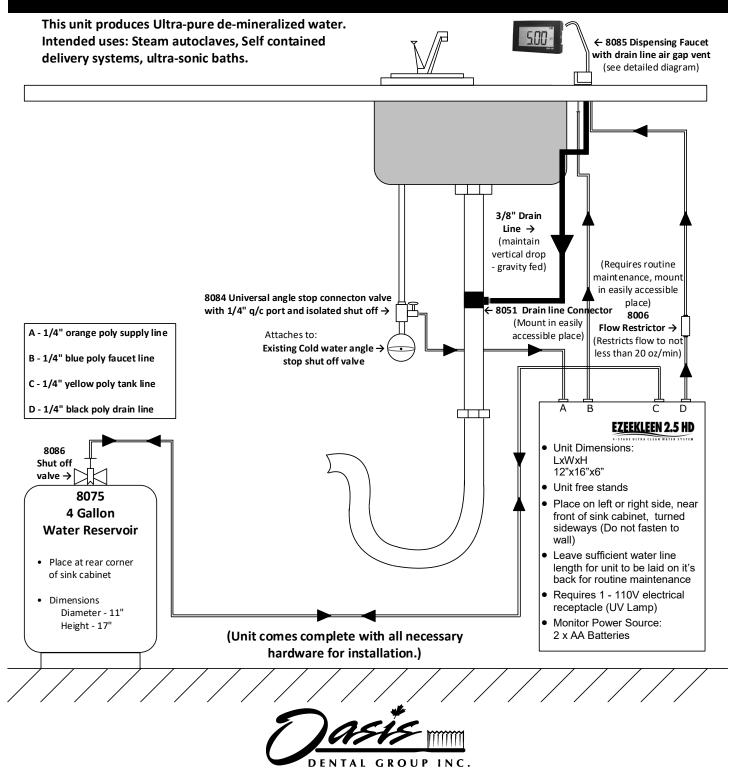


15531 - 24th Avenue, Unit 24, Surrey, BC V4A 2J3 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538 - 1295


© 2009 - 2024 Oasis Dental Group Inc.™

4-STAGE ULTRA CLEAN WATER SYSTEM

Model: 8000

DISPENSING FAUCET WITH DRAINLINE AIR GAP VENT

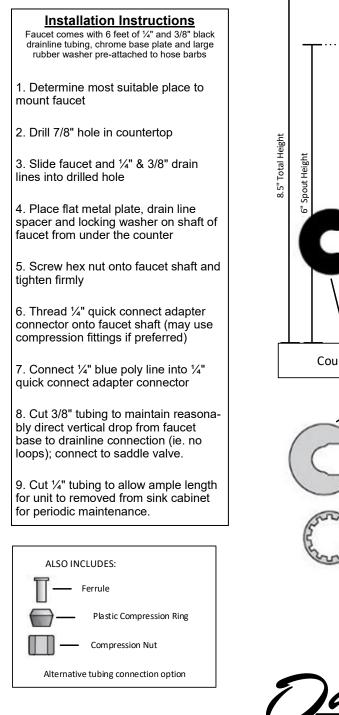

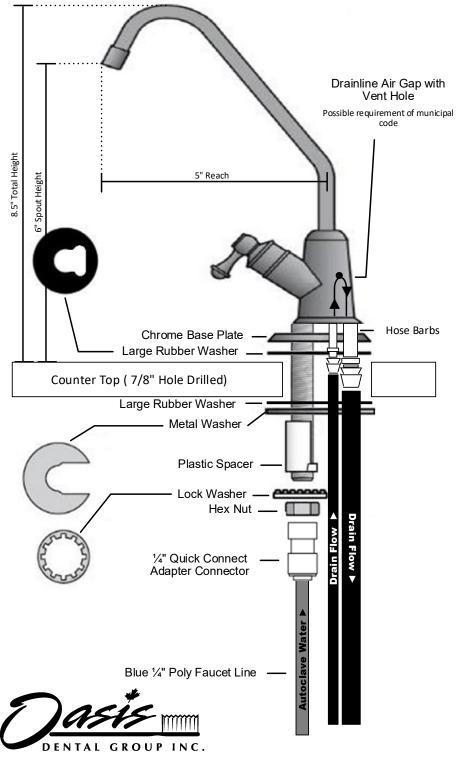

15531 - 24th Avenue, Unit 24, Surrey, BC V4A 2J3 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538 - 1295

© 2009 - 2024 Oasis Dental Group Inc.TM

www.oasisdentalgroup.ca

4-STAGE ULTRA CLEAN WATER SYSTEM

Model: 8000

PROTOCOL FOR USAGE

When drawing water from the Ezee Kleen 2.5 HD ALWAYS ensure the following protocol is used:

- Tip: Photocopy and laminate or contact Oasis Dental Customer Support line for a free laminated copy of this page and post at the Ezee Kleen 2.5 HD dispensing faucet. Do not remove. Update chart each time cartridges are changed.
- Water is suitable for use in autoclaves, self contained dental unit water systems, ultrasonic baths, instrument cleaning and film developers
- Collect and store Ezee Kleen 2.5 HD autoclave safe water in clean containers marked "Autoclave Water Only" "No Tap Water" "Keep Lid On" "Store Only 48 Hours"
- Label the Dispensing Faucet "Autoclave Water Always Check Monitor while Drawing Water"
- Disregard monitor when not dispensing water from the unit (ie. when unit sits idle)
- Check Ezee Kleen 2.5 HD Monitor each time water is drawn to ensure reading is less than 5.0 µS.
- Regularly inspect the containers for cleanliness
- When storing filled containers ensure caps remain on
- Avoid storing or drawing water in an unclean environment
- Avoid storing the water more than 48 hours
- Ensure the working area around the dispensing faucet and especially the dispensing faucet itself remains clean
- Avoid running equipment that has the potential to create dust or particulate matter in the atmosphere when drawing water
- Use "Patient Scheduler" or sign up for our "Annual Maintenance Reminder Program" to schedule maintenance for Ezee Kleen 2.5 HD annually
- See page 11 of user' manual for "Changing your Cartridges Instructions"
- Failure to comply with manufacturer's "Protocol for Usage" and below maintenance recommendations could result in water not suitable for intended use
- Completion of maintenance in accordance with below chart is only maintenance required
- Contact Oasis Dental Group Inc. customer support for any other maintenance

Cartridge	8002-FR DI Cartridge with drainline flow restrictor	Optional 8002-XL DI Cartridge	8003 Pre-Filter	8004 RO Membrane	8005 UV Lamp
Maintenance	Change when monitor reads greater than 5.0 μS with water flowing	Change each time 8002-FR is changed	Change Annually	Change Bi-annually (Every Two Years)	Change Annually
Last maintained					
Changed by					
Cartridge Supplie	r:				
Staff member res	ponsible for maintenance of the	Ezee Kleen 2.5 HD:			

Questions? Contact customer support Mon - Fri, PST, 8:00am - 5:00pm.



15531 - 24th Avenue, Unit 24, Surrey, BC V4A 2J3 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538 - 1295

© 2009 - 2024 Oasis Dental Group Inc.™

www.oasisdentalgroup.ca

4-STAGE ULTRA CLEAN WATER SYSTEM

Model: 8000

CHANGING YOUR CARTRIDGES - INSTRUCTIONS

CHANGING CARTRIDGES BEFORE CHANGING 8002-FR, 8003 or 8004 CARTRIDGE

- A.1 Have a towel available to absorb any water released by system
- A.2 Have full tank of water before changing any cartridges
- A.3 Turn off water supply under sink by closing Ezee Kleen Shut Off Valve or cold water shut off valve
- A.4 Close Ezee Kleen Tank Valve
- A.5 Open Ezee Kleen Dispensing Faucet
- A.6 This will relieve line pressure in the system
- A.7 After completing any cartridge change wait for tank to fill and, with faucet closed, system will be fully pressurized, check for leaks

CHANGE 8003 PRE FILTER CARTRIDGE ANNUALLY

- B.1 Remove Slip-in-Elbow from both ends of cartridge Consult User's Guide to understand quick connect feature on all Ezee Kleen fittings
- B.2 Remove protective dust plugs from new cartridge
- B.3 Replace expired cartridge ensuring water is flowing in the correct direction
- B.4 Reinsert Slip-in-Elbows to both ends of cartridge
- B.5 Turn on water supply
- B.6 Open Ezee Kleen Tank Valve
- B.7 Run water from Ezee Kleen Dispensing Faucet until you have a steady stream of water Continue until tank is empty
- B.8 Close Dispensing Faucet
- B.9 Allow 2 hours for tank to fill again System is now ready to use

CHANGE 8004 REVERSE OSMOSIS (RO) MEMBRANE BI-ANNUALLY (Every 2 years)

- C.1 Disconnect waterlines from all 3 fittings at the ends of RO Cartridge Note which waterline each fitting is attached to
- C.2 Remove RO Cartridge from clips
- C.3 Unscrew cap of RO Cartridge and discard expired RO Membrane
- C.4 Clean inside of RO Cartridge with mild detergent Rinse thoroughly Insert new RO Membrane
- C.5 Screw on RO Cartridge cap Do not over tighten Fit RO Cartridge back into clips
- C.6 Reconnect all 3 waterlines to fittings on RO Cartridge
- C.7 Turn on water supply
- C.8 Open Ezee Kleen Tank Valve
- C.9 Run water from Ezee Kleen Dispensing Faucet until you have a steady stream of water Continue until tank is empty
- C.10 Close Dispensing Faucet
- C.11 Allow 2 hours for tank to fill again System is now ready to use

CHANGE 8005 ULTRA-VIOLET (UV) LAMP ANNUALLY

(Note: UV Lamp can be changed without turning off water)

- D.1 Disconnect power supply to UV Cartridge
- D.2 Swivel/swing UV Cartridge outwards away from unit
- D.3 Grasp white electrical cable exiting end of UV Cartridge
- D.4 Gently pull electrical cable out of UV Cartridge The entire lamp is attached to the electrical cable and will slide out of UV Cartridge
- D.5 Replace UV Lamp by sliding new UV Lamp into the UV Cartridge
- D.6 Re-connect power supply to UV Cartridge

CHANGE 8002-FR DI CARTRIDGE IF MONITOR READING IS GREATER THAN 5.0 μS WHILE WA-TER IS BEING DISPENSED FROM EZEE KLEEN DISPENSING FAUCET

Monitor reading greater than 5.0 μS = water is unacceptable for autoclave use

- E.1 Remove Slip-in-Elbow from both ends of cartridge Consult User's Guide to understand quick connect feature on all Ezee Kleen fittings
- E.2 Remove protective dust plugs from new cartridge
- E.3 Replace expired cartridge ensuring water is flowing in the correct direction
- E.4 Reinsert Slip-in-Elbows to both ends of cartridge
- E.5 Replace 8006 Drainline Flow Restrictor on black 1/4" drainline, <u>on outside of unit</u>, ensuring arrow is pointing away from the unit
- E.6 Turn on water supply
- E.7 Open Ezee Kleen Tank Valve
- E.8 Run water from Ezee Kleen Dispensing Faucet until you have a steady stream of water Continue until tank is empty
- E.9 Check that monitor reading is below $5.0 \ \mu S$
- E.10 Allow 2 hours for tank to fill again System is now ready to use

Call Oasis Dental Group Inc. @ (800) 338-6693, M-F, 8:00 - 5:00 PST for technical assistance.




4-STAGE ULTRA CLEAN WATER SYSTEM

Model: 8000

CONNECTING & DISCONNECTING CARTRIDGES

The Ezee Kleen 2.5 HD is equipped with a unique collet locking system that allows cartridge changes to take only seconds and requires no special training or tools.

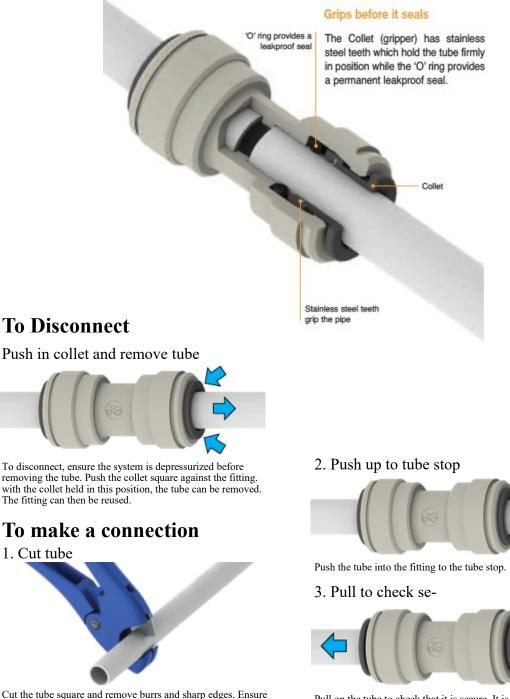

the outside diameter is free of score marks. For soft or thin

Pull on the tube to check that it is secure. It is a good practice to test the system prior to leaving site and/or before use.

© 2009 - 2024 Oasis Dental Group Inc.TM

MAINTENANCE SUPPLIES

TO ORDER YOUR SUPPLIES

1) Contact your authorized **EZEEKLEEN 2.5 HD** dealer. For easy reference, enter your Dealer's name and contact information here:

Or

2) Contact **Oasis Dental Group** at: (800) 338-6693 or (604) 538-1285 Fax: (604) 538-1295 Mail: 16147 - 8A Avenue, Surrey, BC V4A 8W8 Website: www.oasisdentalgroup.ca Email: info@oasisdentalgroup.ca

Ezee Kleen 2.5 HD - Complete Unit - # 8000

De-ionization Cartridge - #8002-FR (includes 8006 flow restrictor)

• change cartridge when monitor reads greater than 5.0 μS <u>with water flowing</u> water is greater than 2.5 PPM (mg/L) of dissolved solids and is unsafe to use in autoclave. Change 8006 Flow Restrictor each time 8002-FR is changed.

XL De-ionization Cartridge (Optional) - #8002-XL

• change cartridge when changing 8002-FR

Prefiltration Cartridge - # 8003

- change annually
- not to exceed 2,000 gallons

Reverse Osmosis Membrane - # 8004

• change bi-annually (every two years)

Ultraviolet Lamp - # 8005

- ultraviolet cartridge will have a noticeable blue illumination when operating. Change the lamp if the illumination ceases, or
- change annually, not to exceed 9,000 hrs of continuous use

Drainline Flow Restrictor—Part #8006

• change when changing 8002-FR DI cartridge

OPTIONAL FEATURES


• XL De-ionization Install Kit - #8002-XL-KIT

- Order for initial XL DI Cartridge install (8002-XL DI Cartridge included)
- Optional tank sizes available
- Total Dissolved Solids Tester (Handheld)
- For water testing contact Oasis Dental Group or a local water testing facility.

4-STAGE ULTRA CLEAN WATER SYSTEM

Model: 8000

INTERNAL DIAGRAM

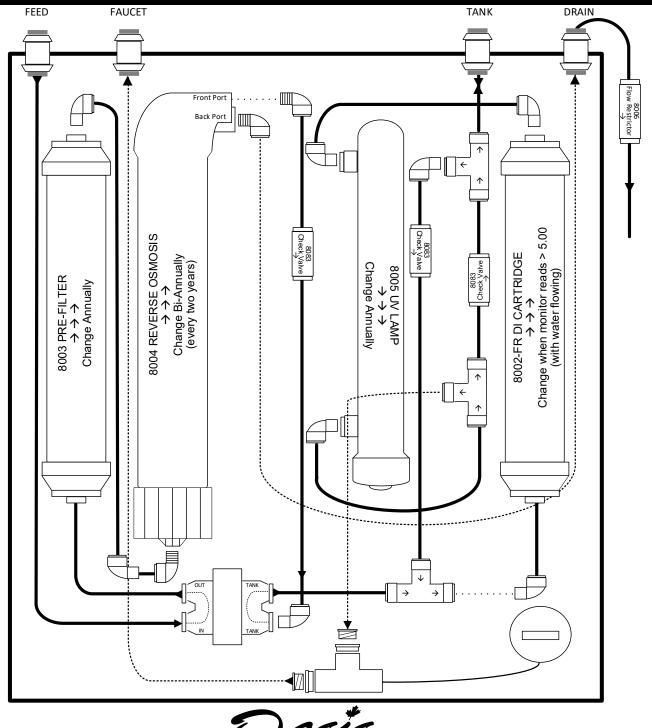



^{15531 - 24}th Avenue, Unit 24, Surrey, BC V4A 2J3 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538 - 1295

 $\ensuremath{\mathbb{C}}$ 2009 - 2024 Oasis Dental Group Inc. $\ensuremath{^{\text{TM}}}$

GUARANTEE/WARRANTY

The EZEEKLEEN 2.5 HD is guaranteed to produce the quality of water necessary to comply with all autoclave/steam sterilizer manufacturer's TDS (total dissolved solids) requirements when used in accordance with manufacturer's directions. Liability is limited to autoclave/sterilizer boiler repair or replacement while under manufacturer's warranty upon given proof manufacturer's TDS requirements have not been met when the EZEEKLEEN 2.5 HD has been used in accordance with manufacturer's (Oasis) directions.

For a period of one year, Oasis Dental Group Inc. guarantees the **EZEEKLEEN 2.5 HD** to be free of defects due to workmanship including all components (with the exception of the De-ionization, Prefiltration, Reverse Osmosis, and Ultraviolet cartridges) when delivered to the customer in new, unused condition by an acknowledged dealer of Oasis Dental Group Inc. products.

In the event of failure due to such defects, within this period of time, the exclusive remedies shall be repair or replacement, at Oasis Dental Group Inc.'s option and without charge, of any defective part(s) provided to Oasis Dental Group Inc. in writing within thirty (30) days of the date of such failure and further provided that the defective part(s) are returned to Oasis Dental Group Inc. freight prepaid.

Any express warranty not provided here on, or any implied warranty or representation as to the performance which may arise by implication not in this provision for the **EZEEKLEEN 2.5 HD** is excluded and disclaimed by Oasis Dental Group Inc.

Warranty Certificate

Keep this and your original invoice of purchase in your permanent records for proof of warranty.

Name:				
Address:				
City:	Province/State:		Postal/Zip:	
Phone Number: ()			
Date of Purchase: Mo:	Day:	Year:		
Dealer's Name:		City:		



15531 - 24th Avenue, Unit 24, Surrey, BC V4A 2J3 • Ph: (800) 338-6693 • (604) 538-1285 • Fax: (604) 538 - 1295

POTABLE WATER QUALITY AND CONTAMINATION PARAMETERS

Sources of Water Contaminants

Sources of drinking water worldwide include rivers, lakes, streams, ponds, reservoirs, springs and wells. As water travels over the surface of the land or through the ground, it dissolves naturally occurring minerals and, in some cases, radioactive material, and can pick up substances resulting from the presence of animals or from human activities. Contaminants that may be present in source water include: microbial contaminants; inorganic contaminants; pesticides and herbicides; organic chemical contaminants; and radioactive contaminants.

Some of the more common sources of substances in water are: erosion of natural deposits, naturally occurring elements, road salt, organic sources such as algae, corrosion of household plumbing systems, leaching from wood preservatives, water additives to promote strong teeth, run-off from fertilizer, decay of natural deposits, man made emissions, leaching from septic tanks, sewage, water softeners, animal waste, soil run-off, by-products of drinking water chlorination, discharge from dry-cleaners, residue from cleaning solvents and metal degreasers, emissions from solvents, chemical intermediates, blowing agents for polyurethane foams, aerosol propellants, fire extinguishing agents, plasticizers from flexible plastics, run-off from herbicide use, human and animal fecal waste, residue from washing detergents, run-off from pesticide use and additives to gasoline in the winter. This list is not necessarily exhaustive.

In order to ensure that tap water is safe to drink, state, provincial and federal health authorities prescribe regulations which limit the amount of certain contaminants in water provided by public water systems. Water quality is monitored over a wide spectrum of microbiological, chemical and physical measures of quality. All public water utilities are required to monitor the quality of water they distribute according to these regulations. Water quality is typically monitored at the source (river, lake, stream, etc.), at the treatment facilities and throughout the distribution system delivering water to the customers point of use.

Drinking water may reasonably be expected to contain at least small amounts of some contaminants. The presence of contaminants does not necessarily indicate that water poses a health risk. More information about contaminants and potential health effects can be obtained by calling, in the United States, the Environmental Protection Agency's Safe Drinking Water Hotline and in Canada, the Health Protection Branch of Health Canada. Contact information can be obtained from your local government authority.

Primary Parameters

Microbiological Guidelines

Microbiological guidelines exist to control the presence of pathogenic or disease-causing micro-organisms. Pathogenic microorganisms that occur in polluted water include protozoa, bacteria and enteric viruses. The most common disease attributable to waterborne pathogenic micro-organisms is gastrointestinal illness or diarrhea. Although gastrointestinal

illness is generally considered to be non-life threatening in normal healthy adults, mortality can occur in sensitive subpopulations, such as infants, the elderly and immunosuppressed individuals. Microbiological guidelines usually establish baseline quantities for total coliforms, faecal coliforms and heterotrophic plate counts or background colony

counts. Normally the guidelines will establish appropriate actions to be taken if baseline quantities are exceeded. Retesting to confirm baseline quantities are not being exceeded is normally expected after corrective action has been taken.

All drinking water supplies should be analyzed routinely for coliform bacteria and the general bacterial population. The presence of excess total coliforms, as stated below, in drinking water indicates that treatment is inadequate or that the distribution system is experiencing re-growth or infiltration. Total coliforms are not necessarily an indication of the presence of fecal contamination. Faecal coliforms in drinking water may, however, indicate the presence of faecal

contamination. The presence of Escherichia coli ("E.coli"), one species in the faecal coliform group, is a definite indicator of the presence of faeces. Other species in the faecal coliform group (e.g. Klebsiella pneumoniae, Enterobacter cloacae) are not restricted to faeces but occur naturally on vegetation and in soils.

The general bacterial population can be estimated from either background colony counts on total coliform membrane filters or heterotrophic plate counts ("HPC"), as outlined in the 16th edition of Standard Methods for the Examination of Water and Wastewater. Excessive concentrations of the general bacterial population may hinder the recovery of coliforms and thereby prevent the detection of a potential threat to public health. Typically the maximum acceptable concentration for coliforms in drinking water is zero organisms detectable per 100mL. Because coliforms are not uniformly distributed in water and are subject to considerable variation in enumeration, authorities typically regulate that drinking water that fulfills the following conditions is considered to be in compliance:

1. No sample should contain more than 10 total coliform organisms per 100 mL, none of which should be faecal coliforms;

2. No consecutive sample from the same site should show the presence of coliform organisms; and

3. For community drinking water distribution systems:

a. not more than one sample from a set of samples taken from the community on a given day should show the presence of coliform organisms; and

b. not more than 10% of the samples based on a minimum of 10 samples should show the presence of coliform organisms.

4. No sample should contain more than 500 HPC colonies per millilitre or more than 200 background colonies on a total coliform membrane filter (i.e. overgrowth)

5. The confirmed presence of E. coli in drinking water should trigger an immediate "boil water advisory".

Recent Outbreaks of Waterborne Infections

Two protozoans of recent particular concern are Giardia cysts and Cryptosporidium oocysts. Outbreaks of Giardiasis occurred in a number of locations in British Columbia and Washington State in the late 1980s. In the spring of 1993 an outbreak of waterborne disease occurred in Milwaukee, Wisconsin, where an estimated 400,000 people became ill with Cryptosporidiosis. Several other North American communities have experienced Cryptosporidiosis outbreaks in the recent past. Cryptosporidiosis, is more serious than Giardiasis as it is untreatable and can cause life threatening illness in those individuals at high risk such as the elderly and those with compromised immune systems. Cryptosporidium is very resistant to the effects of chlorine and therefore water systems with unfiltered surface supplies that rely on chlorination disinfection alone, may be unable to decrease the risk of this disease if significant numbers of the organism are present in the source water.

In May 2000 in Walkerton, Ontario an estimated 2,000 people grew ill from an outbreak of E.coli infection. People became sick with fever, cramps, nausea and bloody diarrhea. Seven people died and an investigation found 1,346 confirmed cases of gastroentreritis were reported to medical officials. It is believed that heavy rain likely washed cattle manure laced with E. coli into one of the town's deep well supplies. Testing of 13 livestock farms near the wells found E. coli on two of them and other bacteria harmful to people on all but two.

These types of outbreaks reinforce the need for adequate disinfection and consistent monitoring throughout public water distribution systems. As an example, the City of New York in 1999 had nearly 1000 fixed sampling stations throughout the city from which it draws samples for monitoring purposes. While not common, waterborne disease outbreaks have occurred and people can be at risk. Again, sensitive subpopulations, such as infants, the elderly and immunosuppressed individuals can be expected to be at greater risk.

Chemical and Physical Guidelines

Guidelines exist to control the presence of chemical and physical elements in public water systems. Chemical and physical elements in public water systems may be undesirable for a number of reasons. Chemicals are normally classified according to data on carcinogenicity. Different approaches are adopted for the derivation of guidelines for compounds considered to be carcinogenic and probably carcinogenic, compounds considered to be possibly carcinogenic and those considered to be probably not carcinogenic or for which data were inadequate for evaluation. Lead poisoning is of particular concern, especially for infants and young children. Water being delivered to public water distribution systems is likely to be leadfree, but water can absorb lead from solder, fixtures, and pipes found in the plumbing of some buildings or homes. Iron, copper and manganese are elements undesirable in water in higher quantities. People on severely restricted sodium diets or moderately restricted sodium diets should concern themselves with sodium levels in public water supplies. Guidelines for chemical and physical parameters are extensive and in some jurisdictions exceed as many as eighty parameters. New parameters are reviewed on an ongoing basis and guidelines undergo continual updates. To determine locally which parameters are monitored and their benchmark guidelines contact the water quality department of your water supply utility and request a "Water Quality Report".

In the United States, the USEPA National Primary Drinking Water Regulations, and in Canada the Health Canada Guidelines for Canadian Drinking Water Guidelines stipulate the parameters and benchmarks for which drinking water must be controlled. Contaminants that may adversely affect public health and occur in drinking water with a frequency and at levels that pose a threat to public health are constantly reviewed. A maximum contaminant level goal is established, below which there is no known or expected risk to health. Next, a maximum contaminant level is established. This is the maximum permissible level of a contaminant in drinking water which is delivered to any user of a public water system. These levels are enforceable standards, and are set as close to the goals as feasible.

Some conventional physical and chemical contaminants that are regulated are antimony, arsenic, asbestos, barium, beryllium, cadmium, chromium, copper, cyanide, fluoride, gross alpha particle, iron, lead, mercury, nickel, nitrate, nitrite, selenium, silver, sulphide, thallium. There are numerous regulated organic contaminants, a few of which are chloramines, dichlorethylenes, tetrachloroethylenes, trichloroethene, and trichlorofluromethanes. Recent attention has been drawn to the chemical MTBE (methyl tertiary butyl ether), an oxygenate widely used as a gasoline fuel additive. MTBE has been found mainly in ground water supplies as a result of leaking gasoline storage tanks and pipelines. The potential for MTBE groundwater contamination is exacerbated by its solubility in water, which allows it to travel through groundwater aquifers faster than the other, less soluble, components of gasoline. The chemical has also been detected at much lower levels in surface water supplies, due more to air emissions and recreational power boating, than to leaking underground storage tanks.

Chlorination of Public Drinking Water Systems

The chlorination of water creates differences in the characteristics of treated water versus raw water. When gaseous chlorine is added to water, it quickly hydrolyzes to form hypochlorous acid and hydrogen and chloride ions. This reaction results in a drop in pH and alkalinity with a subsequent increase in the level of chloride in the water. These changes increase the corrosiveness of water, especially in areas where water may already be corrosive due to natural low pH, low alkalinity and high dissolved oxygen. In these situations it is not uncommon to see at the tap elevated levels of copper and lead, both of which leach from household plumbing. These problems can be further exacerbated in older buildings, particularly buildings with hot water heating systems and galvanized piping.

Chlorination of water supplies, either using liquid chlorine or bleach, leads to the formation of undersirable Disinfection By-Products ("DBP's") through reaction of chlorine with natural organic matter ("NOM") present in raw water. Among the DBP's formed are trihalomethanes ("THM's"), haloacetic acids ("HAA's"), chloral hydrates, haloacetonitriles and chloropicrin. THM's and HAA's are present in significant concentrations in chlorinated waters. Factors affecting the formation of DBP's are chlorine concentration, pH, temperature, bromide, contact time, and the nature and concentration of NOM. NOM consists of total and dissolved organic carbon ("TOC" and "DOC") caused by decaying vegetation in water.

This material has potentially negative effects on water quality. TOC exerts a chlorine demand, that is, chlorine reacts with the organic material in the water resulting in a loss of chlorine residue over time and the production of potentially undesirable DBP's. Chloroform, one THM, is the THM detected most frequently and at highest concentrations in drinking water. Chloroform's volatility creates the potential for exposure to airborne chloroform released from tap water. Available data are consistent with the hypothesis that ingestion of chlorinated drinking water may be causally related to cancers of the bladder and colon. Chloroform has been found to be carcinogenic in two animal species and has been classified as being probably carcinogenic to humans.

Secondary Parameters

Turbidity

Turbidity is a measure of cloudiness of the water. Turbidity is monitored because it is a good indicator of water quality and can hinder the effectiveness of disinfection. Turbidity in water is caused by suspended matter, such as clay, silt, finely divided organic and inorganic matter, soluble colored organic compounds, plankton and other microscopic organisms. Turbidity measurements relate to the optical property of a water that causes light to be scattered and absorbed rather than transmitted in straight lines through the sample. The current method of choice for turbidity measurement is the nephelometric turbidity unit ("NTU").

Excessive turbidity detracts from the appearance, taste and odors of water. It can serve as a source of nutrients for waterborne bacteria, viruses and protozoa, which can be embedded in or adhere to particles in the raw water or become trapped within floc formed during water treatment; turbidity can thus interfere with the enumeration of micro-organisms in finished water, as the microorganisms may not be detectable or may be grossly underestimated by current detection methods. The adsorptive properties of suspended particles can also lead to a concentration of heavy metal ions and biocides in turbid waters. Turbidity can interfere with disinfection processes and the maintenance of a chlorine residue. Turbidity has also been related to trihalomethane formation in chlorinated water. Viable coliform bacteria have been detected in waters with turbidities higher than 3 NTU, even in the presence of free chlorine residuals.

Typically, turbidity guidelines are set at 1NTU for water entering the distribution system (post treatment) and 5 NTU at the point of consumption. However, periodic flushing of the water mains by water utilities may dramatically increase the mains water turbidity for a temporary period.

Hardness

In the United States, the USEPA and in Canada, Health Canada have established a secondary standard for total dissolved solids in public water systems of 500 mg/L. (1 mg/L = 1 PPM). The source of dissolved solids is typically metals and salts naturally occurring in soil and organic matter. Dissolved solids, while not necessarily harmful to humans, contribute to excessive hardness, mineral deposition, corrosion and taste in water.

Water hardness is caused by dissolved polyvalent metallic ions, principally calcium and magnesium, and is expressed as the equivalent quantity of calcium carbonate. Encrustation and excessive soap consumption are the main concerns with hardness. On heating, hard waters have a tendency to form scale deposits. While not typically a regulated parameter, most public water utilities report levels of hardness. Water with 0 - 50 mg/L of hardness is considered soft, between 51 - 151 mg/L is moderately hard and water having (150 mg/L is generally considered to be hard.

PHARMACEUTICAL GRADE WATER

The term pharmaceutical grade water is often used as a collective term for six types of water as defined by the United States Pharmacopeial Convention Inc. ("USP"):

- purified water;
- water for injection;
- bacteriostatic water for injection;
- sterile water for inhalation;
- sterile water for injection; and
- sterile water for irrigation.

Currently USP 23 defines "Purified Water" according to the following monographs:

- pH 5 to 7
- Total Organic Carbons 500 PPB
- Conductivity (µS/cm)
- Stage $1 \le 1.3 \,\mu\text{S/cm}$ (on-or off line; T > 25° C [77°F])
- Stage $2 \le 2.4 \ \mu\text{S/cm}$ (off line; T = 24 to 26° C [75 to 79° F])
- Stage $3 \le 2.4$ to 5.8 μ S/cm (off line; T = 24 to 26° C [75 to 79° F])
- Source water USEPA NPDWR
- Microbiological Concentrations: Recommended "action" limit = 100 CFU/mL.

Water meeting these requirements can be labeled as Pharmaceutical Grade Purified Water. While water of this quality may be desirous it is extremely difficult to obtain and is limited by feasibility. Onsite water purification systems may be able to produce water of this quality by a number of processes but numerous factors will influence the systems ability to maintain production of water of this quality on a consistent and reliable basis. Onsite water purification systems are susceptible to, among other things, source water parameter variations, system performance, system maintenance, operator care and post production handling.

USING YOUR EZEEKLEEN 2.5 HD TO CONTROL WATER QUALITY PARAME-TERS OF CONCERN TO THE DENTAL OFFICE

Water is used in the dental office for a number of purposes beyond that of drinking water. Much of today's dentistry is performed using instruments cooled by water. Specifically, both the high-speed handpiece and the ultrasonic scaler use water as a driving/ cooling agent. The triplex syringe uses water to flush the patients mouth of debris and provide irrigation. Water is commonly used for steam sterilization of instruments. Film developers, ultrasonic baths and instrument cleaning are other sources of water use in the dental office.

Until now the only source of specialized water for the dental office has been purchased water either, through a retail outlet or by a delivery service. The EZEEKLEEN 2.5 HD uses four sophisticated water purification processes to produce an ultra clean quality water. The unit is designed to further process potable water (meeting NPDW regulations) on site, on demand, at an affordable price and eliminates the need to store water in bottles which promote microbiological re-growth. Contaminants taken into consideration in the design of the EZEEKLEEN 2.5 HD include: micro-biological contaminants, inorganic contaminants, pesticides and herbicides, organic chemical contaminants and radioactive contaminants. Water produced may, under certain conditions, meet the definition of Pharmaceutical Grade Purified Water. All of the monographs of USP 23's definition of Purified Water have been taken into consideration in the design of the EZEEKLEEN 2.5 HD.

Parameters outside of the control of the design of the unit are, among other things: source water parameter variations, system maintenance, user care and attention, and post production handling of water produced by the unit. With appropriate protocols and regular testing users may be able to achieve Pharmaceutical Grade Purified Water from their EZEEKLEEN 2.5 HD.

Invasive Procedures and Universal Precautions

Modern dentistry involves many invasive procedures. Many procedures involve the cutting of soft tissue or bone and direct exposure to the patients blood stream. Teeth cleaning predominantly uses ultrasonic scaling to remove stain and tartar high up under the patients gums creating a direct access to the blood stream.

Today's population includes many sensitive subpopulations of greater risk to pathogenic organisms and water contaminants. The use of chemotherapy for cancer treatment has grown enormously creating an immunocompromised group that did not exist only a few decades ago. New treatments for diseases such as cancer, aids, cystic fibrosis, diabetes, etc. are extending the lives of people inflicted with such diseases, but additionally creating new subpopulations of immunocompromised individuals as they live longer. The maturing of North America's baby boom generation is creating an explosion of elderly people more susceptible to compromised immune systems. Modern medicine is helping these people live longer, and as they get older they spend more years in which their immune systems are compromised.

Modern medicine, chemistry and microbiology has made us more aware of other potential risks that were previously unknown. We are now aware of the hazards of lead poisoning coming from the leaching of lead in our household plumbing. Exposure to high levels of copper, manganese and iron are not necessarily desirable. Public water systems high in sodium content may not be appropriate for people on sodium reduced diets. New carcinogens are being discovered daily. It is difficult for the practitioner to have a complete understanding of the patients medical history, thus making it more difficult to identify the patient requiring extra precautions.

More and more practitioners are gaining an appreciation of potential contaminants in municipal water supplies and an understanding of the difficulty public water treatment systems are having in removing and monitoring all of them. Consequently, practitioners may deem it not appropriate to use municipal water in the dental operatory.

Contained Dental Unit Waterline Systems

Bacterial growth and proliferation in dental lines supplying water to high speed handpieces, triplex syringes and ultrasonic scalers has become of recent concern. In North America, the American Dental Association and Canadian Dental Association have both addressed the issue with official position statements. The profession has challenged manufacturers to work towards a goal of no more than 200 colony forming units ("CFU")/mL of water emitted from dental unit waterlines. State and provincial dental associations are starting to address the issue. In the United States, the Occupational Safety & Health Association ("OSHA") has mandated that no more than 200 CFU/mL of legionella should be present in water being emitted from dental waterlines. The Center for Disease and Control is considering updating its guidelines for dental waterlines. Media attention is being drawn to the issue with coverage from such prominent players as ABC's "20/20" Investigative News Program. Studies suggest that few dental waterline systems would meet these guidelines without additional disinfection equipment and/or adequate disinfection protocols. For further information on dental unit water contamination contact Oasis Dental Group Inc. @ 800-338-6693, visit internet site www.safedentalwater.org or contact your state/provincial or federal dental association.

One such potential solution to dental unit water contamination has been the introduction of contained (closed) dental unit water systems which operate independent from the municipal water supplies. These systems provide a reservoir to contain the water supplying the dental unit waterlines. This reservoir allows the user to control the quality of water entering the dental waterlines and provides a point of access to introduce disinfectant products into the system to attempt to control microbiological contamination. These systems also negate the need for backflow preventors on each dental operatory, a common requirement of many municipalities.

The use of EZEEKLEEN 2.5 HD water in contained dental unit water systems offers several benefits. Dental unit water contamination predominantly originates from low levels of bacteria present in municipal water supplies. These bacteria

enter the dental waterlines and adhere to the walls of the waterlines. To survive and multiply the bacteria extract food and nutrients in the form of organic matter and inorganic minerals to develop and build an ecosystem in which they can thrive. EZEEKLEEN 2.5 HD water is processed to minimize microbiological contamination thus minimizing the number of organisms being introduced into the system. Furthermore, EZEEKLEEN 2.5 HD water has little if any organic matter or inorganic minerals present in it, thus minimizing the food supply that bacteria need to build their ecosystem. While using EZEEKLEEN 2.5 HD water alone may not be enough to prevent microbiological growth in dental unit waterlines it will help to reduce the rate of growth and reduce the frequency of chemical treatment protocols on dental waterlines. Reduced chemical treatment means less patient exposure to chemicals, less equipment exposure to harsh chemicals, less staff time performing disinfection protocols on waterlines and less cost on chemical treatment products and protocols.

Another potential solution to dental unit water contamination is the use of microfiltration. Microfiltration cartridges with pore sizes as small as 0.22 micron are available on the market for dental waterlines. While the membranes of these microfiltration cartridges offer a physical barrier to impede the flow of bacteria down the dental waterline they are subject to clogging from two sources: suspended and dissolved solids in municipal water supplies; and, organic growth and bacterial growth in the biofilm in dental waterlines. EZEEKLEEN 2.5 HD water offers a source of water void of the typical suspended and dissolved solids found in municipal water. Secondly, EZEEKLEEN 2.5 HD water has little if any organic matter or inorganic minerals present in it, thus minimizing the food supply for which bacteria need to build their ecosystem. This will assist in retarding the development of biofilm on dental waterlines. Because of these factors, the use of EZEEKLEEN 2.5 HD water will improve the performance and life of dental unit waterline microfiltration cartridges by reducing the level of contaminants with which they are challenged.

Steam Sterilization of Dental Instruments

Steam Sterilization has become the method of choice for sterilizing instruments in the dental office because they offer excellent penetration and relatively short cycles. Water-based liquids can also be sterilized by steam sterilization. There are two types of steam sterilizers common to the dental office: conventional systems; and, cassette-style rapid steam heat. Conventional systems normally operate at 121° C for at least 20 minutes. Cassette-style rapid steam sterilizers normally operate at 135° C for 5 minutes.

Water used in steam sterilizers typically enters a relatively small boiler chamber where it is heated to specified temperatures and evaporates. Instruments are subjected to this heated vaporized steam thereby killing any microbial or viral contaminants present. Impurities in the supply water for the sterilizer, remain in the boiler chamber as a residue. This residue can foul the boiler chamber of a steam sterilizer, shorten it's life and cause it to malfunction or fail completely. Most steam sterilizer manufacturers recommend that water with no more than 5 mg/L of Total Dissolved Solids be used. Additionally, some dissolved solids can be carried with the vaporized water to the instruments and cause pitting, especially on non-stainless steel metals.

The EZEEKLEEN 2.5 HD is designed to provide a very high grade of water suitable for use in all steam sterilizers in the dental office. Water processed by the EZEEKLEEN 2.5 HD has little if any impurities and accordingly, can promote more efficient, effective operation and longer life of the steam sterilizer. Additionally, EZEEKLEEN 2.5 HD water minimizes the risk of instrument pitting from steam sterilization. The EZEEKLEEN 2.5 HD constantly monitors water quality to ensure it has less than 2.5 mg/L of Total Dissolved Solids present.

Ultrasonic Baths, Instrument Cleaning & Film Developers

The EZEEKLEEN 2.5 HD produces an ultra clean quality water free from suspended solids and dissolved solids. These contaminants are often the cause of instrument pitting and deterioration and can potentially influence the quality and clarity of x-rays used in the dental office.

FUNCTION OF EZEEKLEEN 2.5 HD

The EZEEKLEEN 2.5 HD has been designed to further process potable water (meeting NPDW regulations) through four stages of purification to produce a very high grade of water. Each of the stages is described below.

Oasis Pre-Filtration Cartridge. Most municipal water contains chlorine, suspended solids¹ and dissolved organic solids² that may foul Reverse Osmosis (RO) filters and deionization (DI) resins. The Oasis Pre-Filtration Cartridge reduces these contaminants to a level that allows for the proper operation of the RO and DI Cartridges downline in the EzeeKleen 2.5 HD.

Oasis Reverse Osmosis (RO) Cartridge. The Oasis RO Cartridge further removes dissolved organic solids and also reduces dissolved inorganic solids³. After processing by the RO Cartridge, up to 98% of all Total Dissolved Solids (TDS)⁴ have been removed and the water has been prepared for the deionization process.

Oasis Mixed-Bed Deionization (DI) Cartridge. The Oasis Mixed-Bed DI Cartridge uses nuclear grade cation and anion exchange resins to remove the remaining dissolved inorganic solids and dissolved inorganic gases⁵. The cartridge achieves near total ion exchange, providing water with a TDS level of < 2.5 PPM which is ideal for use in all makes of sterilizers (minimum recommended TDS level for sterilizers is < 5 PPM).

Oasis Ultraviolet (UV) Cartridge. The Oasis UV Cartridge produces 32,000 w-sec/cm2 of UV light radiation to destroy bacteria, viruses, algae and yeasts (see page 24 for list of organisms destroyed). The UV radiation destroys an organism by penetrating its cell wall and deactivating its DNA, thereby preventing the organism from reproducing. Removing microbial contamination in this way produces water that is ideal for use in self contained dental unit water line systems, reduces the need for chemical treatment in your dental water lines and reduces the frequency with which you will need to change micro-filtration cartridges.

DEFINITIONS

1 Suspended Solids. Sand, silt, clay particles, grit, dirt, rust and other solid particles that can damage downline equipment.

2 Dissolved Organic Solids. Plant and animal decay and material from human activity. They may include proteins, alcohols, chloramines and residues of pesticides, herbicides and detergents.

3 Dissolved Inorganic Solids. Silicates, chlorates, fluorides, bicarbonates, sulfates, phosphates, nitrates and ferrous compounds.

4 Total Dissolved Solids. Total Dissolved Solids (TDS) is the measurement of the total amount of both organic and inorganic solids dissolved in a sample of water. TDS is measured in mg/L or parts per million ("PPM"). 1 mg/L = 1 PPM.

5 Dissolved Inorganic Gases. CO2 is the most common dissolved inorganic gas and dissolves in water to form weakly acidic carbonic acid (H2CO3).

WATER QUALITY SPECIFICATIONS

COMPARATIVE ASSESSMENT FOR THE REMOVAL OF VARIOUS WATER POLLUTANTS

* some ** most (up to 98%) *** all (100%)

	Activated Carbon/ Sediment Filter	Reverse Osmosis	Di- ionization	Ultraviolet Purification	Ezee Kleen 2.5 HD	Distillation
Sodium		**	***		* * *	**
Arsenic		**	***		***	**
Lead		**	***		* * *	**
Cadmium		**	***		* * *	**
Potassium		**	***		***	**
Sulfates		**	***		***	**
Calcium (Hardness)		**	***		***	**
Magnesium (Hardness)		**	* * *		* * *	* *
Phosphates		**	***		***	**
Fluorides		**	***		***	**
Alkalinity		**	***		***	**
Fecal Bacteria	*	**		* * *	***	**
Viruses		**		* * *	***	**
Organics	**	**		* * *	***	*
Trihalometheses (THM)	* *	***			* * *	*
Trichlorsethylene (TCE)	**	***			***	*
Dioxin	*	***			* * *	*
Radioactive Con- taminants		**	***		* * *	* *
Chlorine	**	***			***	*
Pesticides	**	***			***	**
Sediments	**	***			***	**
Unpleasant taste/ odor	**	***			* * *	

WATER QUALITY SPECIFICATIONS

The **EZEEKLEEN 2.5 HD** effectively uses Ultraviolet (UV) radiation to destroy bacteria, viruses and other microorganisms by interfering with the DNA and RNA in the organisms' reproductive cycles. The contact disinfectant property of UV radiation energy is measured in microwatt-seconds per square centimeter (w-sec/cm2). The **EZEEKLEEN 2.5 HD** produces 32,000 to 35,000 (w-sec/cm2).

BACTERIA

Agrobacterium	8,500
Bacillus anthracis	8,700
Bacillus megaterium (vegetative)	2,500
Bacillus subtilis (vegetative)	11,000
Clostridium tetani	22,000
Corynebacterium diphtheriae	6,500
Escherichia coli	7,000
Legionella bozemanii	3,500
Legionella dumoffii	5,500
Legionella gormanii	4,900
Legionella micdadei	3,100
Legionella longbeachae	2,900
Legionella pneumophila	3,800
Leptospira interrogans (Infectious Jaundice)	6,000
Mycobacterium tuberculosis	10,000
Neisseria catarrhalis	8,500
Proteus vulgaris	6,600
Pseudomonas aeruginosa laboratory strain	3,900
Pseudomonas aeruginosa environmental strain.	10,500
Rhodospirillium rubrum	6,200
Salmonella enteritidis	7,600
Salmonella paralyphi (Enteric Fever)	6,100
Salmonella typhimurium	15,200
Salmonella typhosa (Typhoid Fever)	6,000
Sarcinia lutea	26,400
Serratia marcescens	6,200

BACTERIA, continued

Shigella dysenteriae (Dysentery)	4,200
Shigella flexneri (Dysentery)	3,400
Shigella sonnei	7,000
Staphylococcus epidermidis	5,800
Staphylococcus aureus	7,000
Streptococcus faecalis	10,000
Streptococcus hemolyticus	5,500
Streptococcus lactis	8,800
Viridans streptococci	3,800
Vibrio cholerae	6,500

ALGAE

Chlorella vulgaris	(algae)	
--------------------	---------	--

VIRUSES

Bacteriophage (E.coli)	6,600
Hepatitus virus	8,000
Influenza virus	6,600
Poliovirus (Poliomyelitis)	21,000
Rotavirus	24,000

YEAST

Baxter's yeast	8,800
Brewer's yeast	6,600
Common cake yeast	13,200
Saccharomyces var. ellipsoideus	13,200
Saccaromyces sp	17,600

ANALYTICAL REPORT ON EzeeKleen 2.5 HD WATER

Norwest		Analytical Report			9938-67 Avenue Edmonton, AB. T6E 0P5 Phone: (780) 438-5522 Fax: (780) 438-0396			
Agri-Food & Environmental Group Calgary Edmonton Winnipeg Lethbridge Sur	rey							
Client: Oasis Dental Group In	c.	Project ID	le.		NWL L	ot ID:	70514	
16147 8A Avenue Surrey, BC., V4A 8W8 Attn: Todd Klymchu Sampled By:	3	Name: Location: LSD: P.O.: Acct. Code:	Easy Clean		Date R Date R	l Number: Received: Reported: Number:	Dec 14, 1999 Jul 13, 2000	
					Page:		1 of 4	
	S	WL Number: ample Date: ample Description:	70514-1 Easy Clean 2.5	5				
Analyte		Units	Results	, ,				
Metals Dissolved Aluminum	Dissolved		-0.008					
	Dissolved	mg/L	< 0.008					
Antimony Arsenic	Dissolved	mg/L mg/L	<0.005 <0.01					
	Dissolved	mg/L	<0.0002					
	Dissolved	mg/L	<0.0005					
Bismuth	Dissolved	mg/L	<0.007					
Boron	Dissolved	mg/L	<0.002					
Cadmium	Dissolved	mg/L	<0.0005					
Chromium	Dissolved	mg/L	<0.0008					
Cobalt	Dissolved	mg/L	<0.0007					
Copper	Dissolved	mg/L	<0.001					
Lead	Dissolved	mg/L	<0.002					
Lithium	Dissolved	mg/L	<0.001					
Molybdenum	Dissolved	mg/L	<0.001					
Nickel	Dissolved	mg/L	<0.001					
Phosphorus	Dissolved	mg/L	<0.03					
Selenium	Dissolved	mg/L	<0.004					
Silicon	Dissolved	mg/L	<0.004					
Silver	Dissolved	mg/L	<0.001					
Strontium	Dissolved	mg/L	0.0003					
Sulphur Thallium	Dissolved Dissolved	mg/L	<0.008					
Tin	Dissolved	mg/L mg/L	<0.004					
Titanium	Dissolved	mg/L	0.0013					
Vanadium	Dissolved	mg/L	<0.001					
Zinc	Dissolved	mg/L	0.0050					
Microbiological Analysis								
Heterotrophic (Standard) Plate Count - Aerobic	Pour Plate	CFU/mL	1					
Physical and Aggregate Prope	erties							
Solids	Total Dissolved	l mg/L	<1.0				-	
Turbidity		NTU	0.15					
Temperature of observed pH	_	°C	-					
Colour	True	Colour units	3					
Carbon Dioxide		mg/L	<5					

ANALYTICAL REPORT ON EzeeKleen 2.5 HD WATER

Norwest		Analytical Report		Edmonton, A Phone: (74	1 /	
Agri-Food & Environmental Group Calgary Edmonton Winnipeg Lethbrid	ge Surrey					
Client: Oasis Dental Group Inc. 16147 8A Avenue Surrey, BC., V4A 8W8 Attn: Todd Klymchuk Sampled By:		Project ID: Name: Easy Clean Location: LSD: P.O.: Acct. Code.		NWL Lot ID:70514Control Number:Date Received:Date Received:Dec 14, 1999Date Reported:Jul 13, 2000Report Number:89744		
				Page:	2 of 4	
		NWL Number: Sample Date: Sample Description:	70514-1 Easy Clean 2.5			
Analyte		Units	Results	·		
Routine Water						
pH Conductivity Calcium Magnesium Sodium Potassium Iron Manganese Chloride Fluoride Nitrate and Nitrite - N Sulphate Hydroxide Carbonate Bicarbonate P-Alkalinity T-Alkalinity Hardness	Dissolved Dissolved Dissolved Dissolved Dissolved Dissolved	uS/cm mg/L mg/L mg/L mg/L mg/L mg/L mg/L mg/	. <5			
	s is a replacemen	-		etals scan, there is no charg	e for this report. Mike	
				Approved by:	2	
Salue Accredited by t	he Standards Cour	ncil of Canada (SCC) and b	y the Canadian Associatio	n for Environmental Analytical I	_aboratories	

ANALYTICAL REPORT ON EzeeKleen 2.5 HD WATER

Easy Clean

Page:



Agri-Food & Environmental Group Calgary Edmonton Winnipeg Lethbridge Surrey Client: Oasis Dental Group Inc.

16147 8A Avenue

Surrey, BC., V4A 8W8

Attn: Todd Klymchuk

Methodology and Notes

Project ID:

Name:

LSD:

P.O.:

Location:

Acct. Code:

9938-67 Avenue Edmonton, AB. T6E 0P5 Phone: (780) 438-5522 Fax: (780) 438-0396

NWL Lot ID:	70514		
Control Number:			
Date Received:	Dec 14, 1999		
Date Reported:	Jul 13, 2000		
Report Number:	89744		

3 of 4

Method of Analysis:

Sampled By:

Test	Reference	Method	Date of Analysis	Location	Analyst
Alkalinity, pH, and EC in water	АРНА	Electrometric Method, 4500-H+ B	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
		Laboratory & Field Methods, 2550 B	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
. e		Laboratory Method, 2510 B	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
		Titration Method, 2320 B	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
Anions (Routine) by	APHA	Single-Column Ion	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
Ion Chromatography		Chromatography with Electronic Suppression, 4110			
		С			
Chloride in Water	АРНА	Automated Ferricyanide Method, 4500-Cl- E	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
Colour (True) in water	АРНА	Visual Comparison Method, 2120 B	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
Fluoride in water	АРНА	Ion Selective Electrode, 4500-F-C	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
Heterotrophic	APHA	Heterotrophic Plate Count -	Jul 12, 2000	Norwest Calgary	Micheal Yohemas
(Standard) Plate Count (Aerobic PP)		Pour Plate Method, 9215 B			
Metals Trace	АРНА	Inductively Coupled Plasma	Jul 13, 2000	Norwest Edmonton	Lang Que Tran
(Dissolved) in water		(ICP) Method, 3120 B	,		
Solids Dissolved	APHA	TDS Dried at 103-105 C,	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
(Total, Fixed and		2540 C			
Volatile)					
Turbidity in Water	АРНА	Nephelometric Method, 2130 B	Jul 12, 2000	Norwest Edmonton	Micheal Yohemas
	· · · · · · · · · · · · · · · · · · ·				

Accredited by the Standards Council of Canada (SCC) and by the Canadian Association for Environmental Analytical Laboratories (CAEAL) for specific tests registered with the Council and the Association

* APHA Standard Methods for the Examination of Water and Wastewater